


Mod. 50

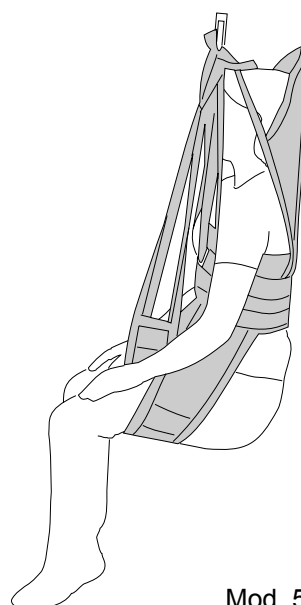

Mod. 55

Product Description

This instruction guide is valid for Liko HygieneVest and "TeddyVest" Hygiene, but in the following text we will only use the name Liko HygieneVest.

Liko HygieneVest is designed for safe lifting and transfer to and from the toilet.

In terms of function and safety, the HygieneVest offers unique advantages and works well in complicated problem situations where no other alternatives are appropriate. The HygieneVest has an outer vest section that surrounds and firmly supports the upper body during lifting. A generous opening around the seat leaves much of the lower body free for dressing and undressing during the actual lifting operation in connection with visits to the toilet.

Liko HygieneVest is the preferred choice of many patients because it enables a stable, upright sitting posture. HygieneVest can also be the best choice for severely functionally disabled amputees or those who have problems with spasticity (best choice, Mod. 55).

Even patients with limited torso stability and poor muscle tone can usually manage lifts with the HygieneVest, and they find it secure and comfortable.

The HygieneVest is intended for sit-to-sit lifting.

The sitting posture is almost fully upright, which facilitates lifts to the toilet and positioning in a wheelchair.

Since the HygieneVest is not placed over the hips, it is ideal for lifting to and from custom-moulded seats and close-fitting wheelchairs.

Liko HygieneVest in sizes XXS and XS are made of a Teddy bear patterned Polyester fabric and this is why these slings are called "TeddyVest" Hygiene. In these sizes, the leg supports are reinforced and padded with a teddy bear patterned polyester fabric. Slings in sizes S to XXXL are made of green polyester and the leg supports are reinforced and padded with a curduroy fabric.


These material combinations apply to the same sizes in model 55.

Liko HygieneVest High Back, Mod 55/ "TeddyVest" Hygiene High Back, Mod. 55


Liko HygieneVest with High Back is the right choice for those who need support to prevent the head from tilting back. For patients who have problems with spasticity, try Model 55.

△ "Caution!" triangles are used to warn of situations that demand extra care and attention.

In this document, the person being lifted is referred to as the "patient" and the person helping them is referred to as the "caregiver".

 Before using lifts and lifting accessories, read the instructions for both the sling and the lift that will be used. Instruction guides can be downloaded, free of charge, at www.liko.com.

Liko HygieneVest

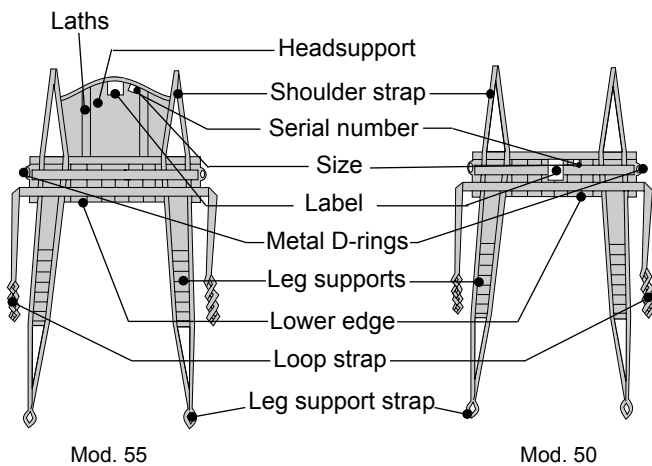


△ Before lifting, remember the following!

- The need for one or more caregivers must be determined from case to case.
- Plan the lift carefully to ensure that it is performed as safely and conveniently as possible.
- Although Liko's slingbars are equipped with safety latches, particular care must be taken. Before the patient is lifted from the underlying surface, but after the straps have been fully extended, make sure the straps are properly hooked to the slingbar.
- Never lift a patient higher above the underlying surface than is necessary for the lifting and transfer procedure.
- Check to ensure that the patient is sitting securely in the sling before starting the transfer.
- Never leave a patient unattended during a lifting situation.
- Make sure the wheels on the wheelchair, bed, gurney, etc. are locked during the lifting/transfer operation.

Transfer from wheelchair to toilet


Prepare to undress the patient by undoing buttons and zippers.

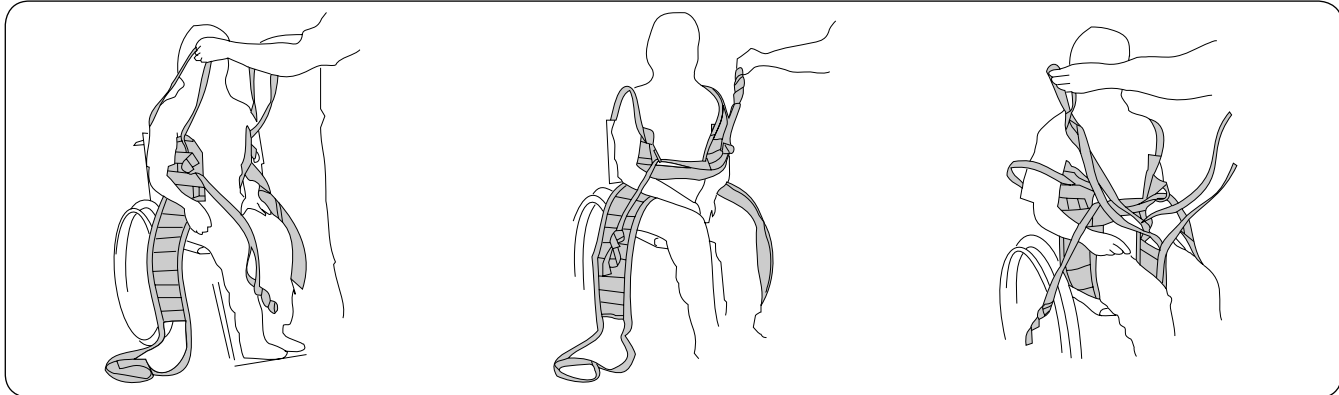

Place the vest around the patient, with the label facing out. Put the arms through the shoulder straps.

Draw the right loop strap through the left D-ring. Draw the left loop strap through the right D-ring.

Position the leg supports under the patient's thighs and cross the leg support straps.

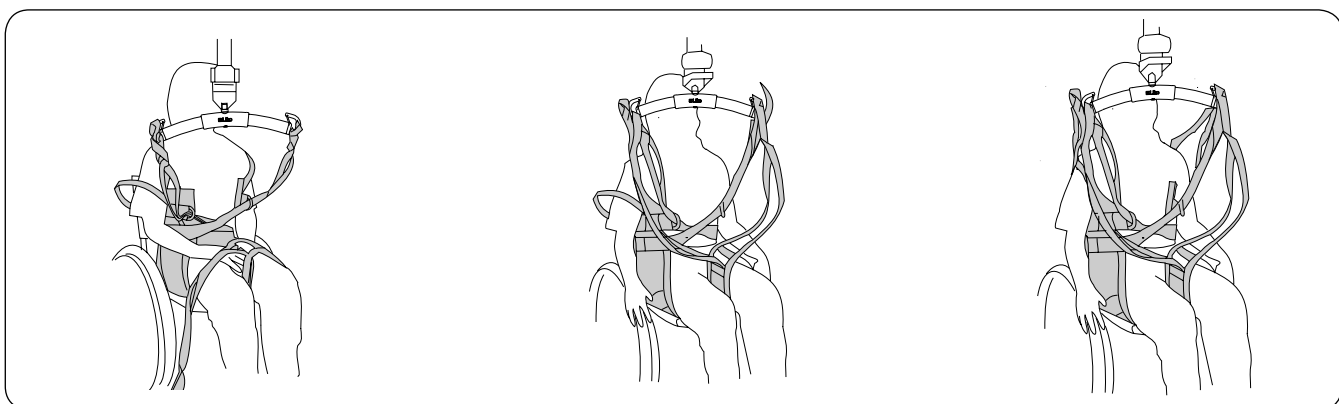

Connect the loop straps to the slingbar at the appropriate loop; see page 4.


Connect the crossed leg support straps to the slingbar. There are two alternatives, see page 4.

Finally, connect the shoulder straps to the slingbar.

△ Important!

The HygieneVest is intended for sit-to-sit transfers. If it is used for lifting from a horizontal position, the shoulder straps will wear out faster.

The shoulder straps should always be connected last to the slingbar.

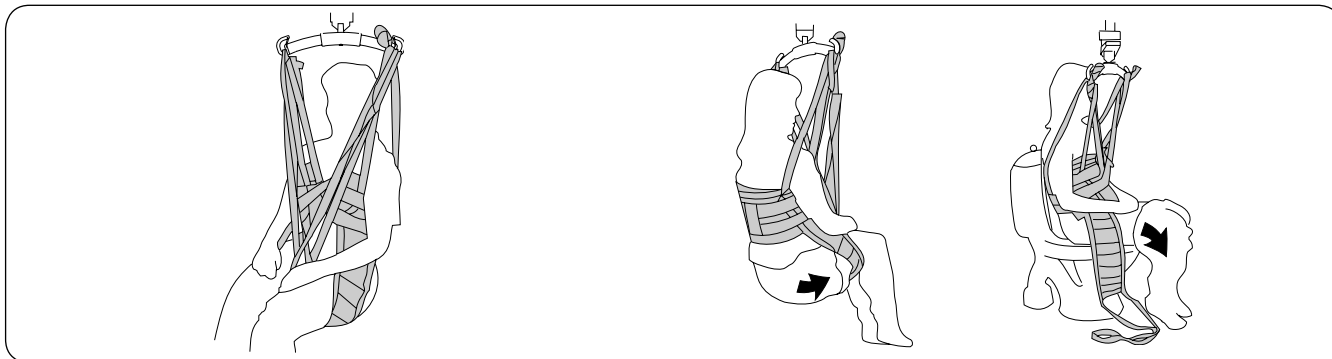

Carefully raise the lift. Make sure the pressure is comfortably distributed around the upper body. If not, lower the sling and make the appropriate adjustments. See page 4.

Pull the clothing down as far as possible and lower the patient to the toilet. Disconnect the leg supports and lower the clothing further.

The vest section can remain around the upper body for support.

In some cases, it may be easiest to leave the leg supports connected during visits to the toilet (applies mainly to female patients).

Return transfer from toilet to wheelchair

Described below are two ways of dressing the patient after a toilet visit.

The most appropriate alternative depends on the patient's condition and type of clothing.

Alternative 1: Leg supports outside the garments. Appropriate for patients with non-elastic pants.




Draw the pants up as close to the crotch as possible.

Position the leg supports under the thighs but outside the pants. Connect all loop straps (see page 2). Lift.

If needed, place an incontinence pad inside the pants before you draw them over the hips. Transfer the patient and lower him/her into the wheelchair.

Alternative 2: Leg supports inside – pants outside. This method is appropriate for patients with elastic pants.

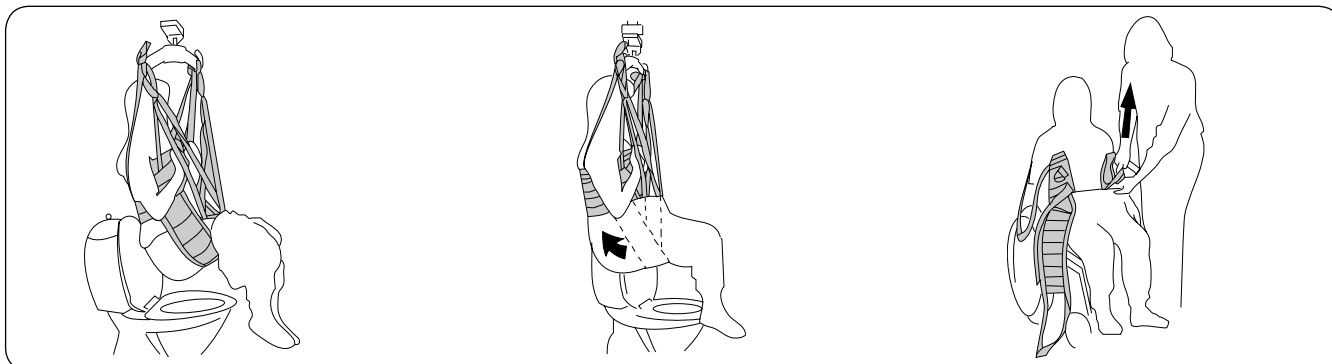

Connect all loop straps (see page 2). Lift. An incontinence pad can be placed inside the crossed leg supports.

Pull the pants up over the hips and leg supports while the patient is sitting in the sling. Transfer the patient to the wheelchair.


Disconnect the strap loops. Carefully work the leg supports out of the pants and remove the HygieneVest.

Fitting instructions


It is essential that the HygieneVest's width is correct in relation to the girth of the patient's upper body. Distribution of pressure around the chest varies according to slingbar width. Try different variations.

Selecting the right size

Check the size of the gap between the front edges of the vest when it is closed. The gap varies depending on the size of the vest, but it should be between 5 and 30 cm (2-12 inch.). The larger the size, the wider the gap can be.

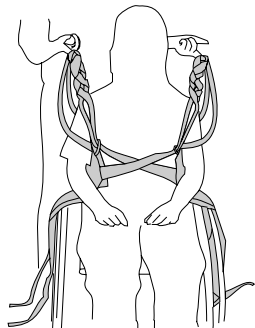

Too small. The gap is too wide and the loop straps are shorter than the shoulder straps when suspended.

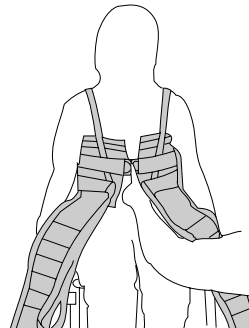

Too large. The metal D-rings meet and the vest cannot be tightened enough with the loop straps.

Adjusting the loop straps



The tension of the vest around the chest is determined by which loop you attach to the slingbar. By test lifting using different loops together with the shoulder straps, you can determine which position gives the right degree of tension.

If the vest slides up - try an inner loop or a smaller sized vest.

If the vest is too tight around the chest - try an outer loop or a larger sized vest.


For a slender person, you would need to use an inner loop and for a heavier person, you would need to use an outer loop if both were using the same size of vest.

When loop straps are properly adjusted, the shoulder straps and loop straps are equally taut during lifting.

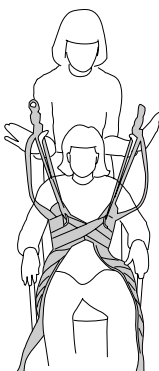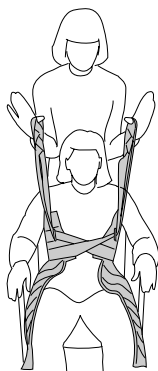


Testing loop strap adjustments

Stand behind the patient and hang the shoulder straps and loop straps on your thumbs. Lift until the straps are fully suspended. If properly adjusted, the shoulder straps and loop straps will be equally taut.

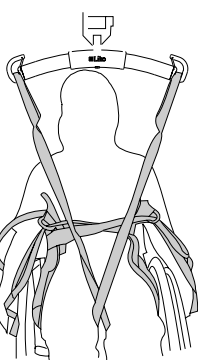

Gives an upright sitting position. Suitable for most patients.

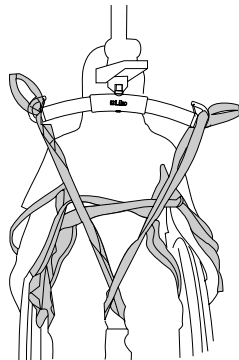

Suitable for shorter patients.

Adjusting the leg supports


Generally, the leg supports are adjusted according to the height of the patient. For a shorter person, attach the leg supports' inner loops to the slingbar. This usually enables a more reclined sitting position.

Try different alternatives until you find the best one.

Helpful hint: Instead of connecting the inner loop, try knotting the leg support strap loops.

Positioning the leg supports

△ How well the patient sits in the sling is determined by **where** you place the leg supports under the thighs. For a patient with weak muscles, place the leg supports as close to the crotch as possible so he/she does not sink down in the sling.

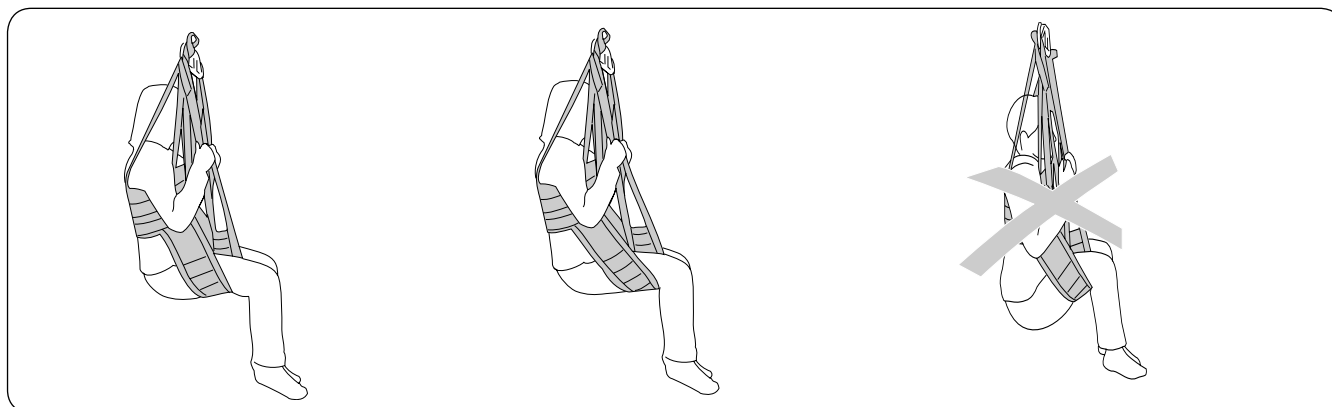

Correct positioning of leg supports for most patients.

For patients with good muscle tone, it may be better to place the leg supports closest to the knee.

If the patient sinks down in the sling and is uncomfortable, the leg supports should be placed closer to the crotch.

Helpful hints:



If you have test fitted a HygieneVest on a relatively slender patient according to the instructions on page 4, but find the vest is still too loose, try crossing the loop straps once (above the D-rings), as illustrated, before attaching the loop straps to the slingbar.

For some patients, e.g. amputees, it may be helpful to pull the leg support loops inside the crossed loop straps, or through the metal D-rings, before attaching them to the slingbar. This prevents the leg supports from sliding forward on the legs.


Accessories

Padded case

Prod. No. 3666021


Padded cases are available as an accessory to help relieve pressure on the front shoulder straps.

Padded cases are equipped with a velcro strip along one side for easy application.



Loop Clips


This practical accessory is used to mark the loops that have been tried out for a certain person. It makes it easier for the caregivers to choose the right loop to attach to the slingbar.

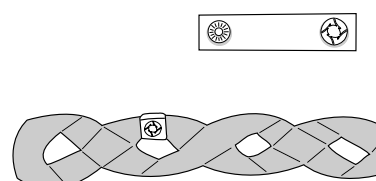

Overview, Liko HygieneVest, Mod. 50, 55



Model 50



Model 55

Product	Prod. No.	Prod. No.	Size	Body weight*	Maximum load**
"TeddyVest" Hygiene	3550812	3555812	XXS	< 20 kg (< 44 lbs.)	200 kg (440 lbs.)
"TeddyVest" Hygiene	3550813	3555813	XS	20-40 kg (44-88 lbs.)	200 kg (440 lbs.)
Liko HygieneVest	3550114	3555114	S	30-60 kg (66-132 lbs.)	200 kg (440 lbs.)
Liko HygieneVest	3550115	3555115	M	50-80 kg (110-176 lbs.)	200 kg (440 lbs.)
Liko HygieneVest	3550116	3555116	L	70-100 kg (154-220 lbs.)	200 kg (440 lbs.)
Liko HygieneVest	3550117	3555117***	XL	90-130 kg (198-286 lbs.)	300 kg (660 lbs.)
Liko HygieneVest	3550118	3555118***	XXL	130- kg (286- lbs.)	300 kg (660 lbs.)
Liko HygieneVest	3550119		XXXL	150- kg (330- lbs.)	300 kg (660 lbs.)

* NOTE! Indicated weights are just guidelines. Deviations may occur.

** Sling sizes Extra Extra Small up to Large are load tested for up to 200 kg (440 lbs.).

Sling sizes Extra Large up to Extra Extra Extra Large are load tested for up to 300 kg (660 lbs.).

*** Made to order Sling.

355-15 → Size
 0 Liko HygieneVest
 5 Liko HygieneVest High Back

Order number example: Prod. No. 3550115

Liko HygieneVest, polyester, medium.

Laundering: See the sling's product label.

Recommended combinations of Liko HygieneVest and Liko's slingbars:

		Mini 220	Slim 350	Universal 350	Standard 450	Universal 450	Wide 670	Twinbar 670
"TeddyVest" Hygiene, XXS	50, 55	1	1	1	1	1	3	4
"TeddyVest" Hygiene, XS	50, 55	1	1	1	1	1	3	4
HygieneVest, S	50, 55	1	1	1	1	1	3	3
HygieneVest, M	50	2	1	1	1	1	2	2
HygieneVest, L	50	2	1	1	1	1	2	2
HygieneVest, XL	50	3	2	1	1	1	2	2
HygieneVest, XXL	50	4	3	2	1	1	1	1
HygieneVest, XXXL	50	4	3	3	1	1	1	1
HygieneVest High Back, M	55	2	1	1	1	1	3	3
HygieneVest High Back, L	55	2	1	1	1	1	2	3
HygieneVest High Back, XL	55	3	2	2	1	1	3	3
HygieneVest High Back, XXL	55	3	2	2	1	1	3	3

Code:

- 1 Recommended
- 2 Possible
- 3 Not advisable
- 4 Inappropriate

The above table summarizes the recommendations for each size. Different slingbar sizes will result in different degrees of pressure around the chest. Test various sizes until you find the most appropriate one.

Combinations with Liko HygieneVest and Cross-bar, Cross-bar 450/670 or Side bars is not appropriate.

CE Medical technical Class I product

Liko HygieneVest has been tested by an accredited test institute and complies with all requirements for MDD Class-I products and the harmonized standard EN ISO 10535.

Liko's products are constantly being updated and refined. Liko reserve the right to change aspects of the products without prior notice. Contact your local Liko representative for updated information and advice.

△ Important!

Lifting and transferring a patient always involves a degree of risk. Study the instruction guides for both lift systems and accessories carefully. A complete understanding of the contents of instruction guides is essential. Only trained personnel should use the equipment. Make certain that the lift accessories are appropriate for the lift you are using and for the lifting situation. Exercise caution and care when using lift equipment and accessories.

As a caregiver, you are responsible for the patient's safety. You must be well informed of the patient's condition and ability to manage the lifting situation. Inspect the sling regularly, especially after laundering. Check carefully for wear and damage to seams, fabric, straps and strap loops. Never use damaged accessories! When in doubt, contact the manufacturer or supplier.

LIFTS WITH CARE



www.liko.com

Manufacturer:

Liko AB
 SE-975 92 Luleå
 Sweden
 info@liko.se

Liko Distributor in USA and Canada:

Liko North America • 122 Grove Street
 Franklin, Ma 02038, USA
 Phone: 508-553-3993, 1-888-545-6671
 Fax: 508-528-6642
 info@liko.com

Liko Distributor in UK:

Liko (UK) Ltd. • Brunel Centre,
 Stroudwater Business Park,
 Stonehouse, Gloucester
 GL10 3RU, United Kingdom
 Phone: +44 (0) 1453 827272
 Fax: +44 (0) 1453 828844
 info@liko.co.uk

